



**HD2013**  
**HD2013UA**  
**HD2013UD**

► [ GB ] Tipping bucket  
rain gauge



## TIPPING BUCKET RAIN GAUGE



The HD2013 is a reliable and sturdy tipping bucket rain gauge, built entirely from corrosion resistant materials in order to guarantee its durability. So as to ensure accurate measurement even with low temperature climatic conditions or during and after precipitations of snow, a version with heating which is automatically activated around +4 °C has been developed so that snow deposits and ice formations are prevented.

The rain gauge is formed by a metal base on which a tipping bucket is set. The rain collector cone, fixed to the aluminium cylinder, channels the water inside the tipping bucket: once the predefined level is reached, the calibrated bucket rotates under the action of its own weight, discharging the water. During the rotation phase, the normally closed reed contact opens for a fraction of a second, sending an impulse to the counter.

The quantity of rainfall measured is based on the count of the number of times the bucket is emptied: the reed contacts, normally closed, open at the moment of the rotation between one bucket's section and the other. The number of impulses can be detected and recorded by a **data logger such as the HD2013-DB** Delta OHM or by a pulse counter.

The rain gauge is available with **optional analog output (HD2013UA)** at choice between 4...20 mA or 0...10 Vdc (**to be specified when ordering**) or with **optional SDI-12 digital output (HD2013UD)**.

The version with 4...20 mA output and the version with SDI-12 output require 7...30 Vdc power supply. The version with 0...10 Vdc output requires 13...30 Vdc power supply. The versions with analog or SDI-12 output are equipped with a backup battery that allows maintaining the rainfall information even after short power supply outages (**at least 10 seconds for HD2013UA, approx. 5 minutes for HD2013UD**).

A removable filter for periodic cleaning and maintenance is inserted in the water collector cone so as to prevent leaves or other elements blocking the end of the hole.

For a better water flow, the collecting cone is treated with a non-adherent product.

In the version with heating HD2013R, the heating circuit operates with 12 Vdc or 24 Vdc direct voltage (**to be specified when ordering**) and absorbs about 165W. Heating is activated around +4 °C.

**When submitting your order**, upon request a bird dissuader, made of eight 3 mm diameter spikes, 60 mm in height, can be installed on the rain gauge.

## Technical characteristics

	HD2013R	HD2013	HD2013UA analog output option	HD2013UD SDI-12 output option
Power supply	Heating circuit: 12 or 24 Vdc ± 10% (to be specified when ordering)	---	7...30 Vdc (4...20 mA output) 13...30 Vdc (0...10 V output)	7...30 Vdc
Consumption	165 W	---	26 mA max. @ 18 Vdc (4...20 mA version) ≈ 4 mA @ 18 Vdc (0...10 V version)	≈ 100 µA @ 18 Vdc in SDI-12 mode
Contact output	NC contact (opens during tipping). With HD2013UA and HD2013UD options, the contact output is alternative to the analog or SDI-12 output and <b>the rain gauge is factory-configured with analog (HD2013UA) or SDI-12 (HD2013UD) output.</b>			
Analog output	---	---	4...20 mA or 0...10 V (to be specified when ordering)	---
Digital output	---	---	---	SDI-12
Resolution	0.1 – 0.2 or 0.5 mm/tip on request when ordering			
Accuracy	See the typical <b>normalized</b> curve in fig. 1. The curve is normalized to the resolution 0.200 mm/tip @ 50 mm/h. If the HD2013-DB data logger is used, the measurement can be automatically corrected according to the curve. With HD2013UA and HD2013UD options, the curve can be stored in the rain gauge itself <b>(on request when ordering)</b> .			
Operating temperature	-20...+60 °C	+4...+60 °C		
Heating intervention temperature	+4 °C	---		
Protection degree	IP 64			
Collector area	400 cm²			
Minimum section of the wires of the connecting cable	0.5 mm² for the version without heating (HD2013) 2.5 mm² for the version with heating (HD2013R)			



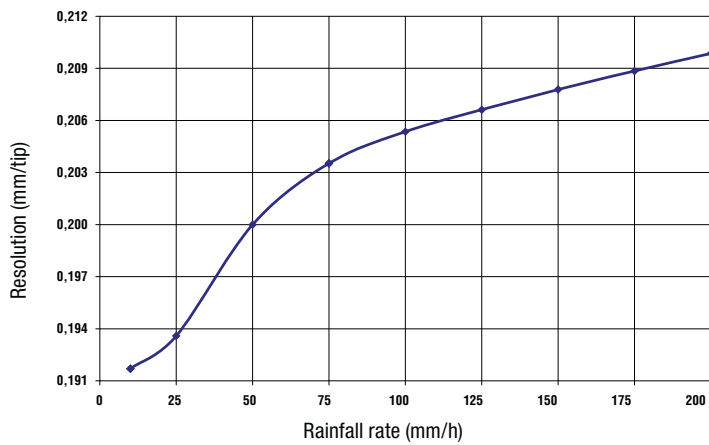


Fig. 1 – Resolution as a function of the rainfall rate

## Installation

Upon request the rain gauge can be supplied already calibrated at 0.1 - 0.2 or 0.5 mm of rain per tip of the bucket: the calibration value is shown on the instrument label.

The instrument must be installed in an open area, away from buildings, trees, etc., ensuring the space over it is free from all objects which could obstruct rain measurements, and in an easily accessible position for the filter to be cleaned periodically.

Avoid installation in areas exposed to gusts of wind, turbulence (for example the top of a hill) as these may distort the measurements.

The rain gauge can be installed on the ground or raised 500 mm above the ground. Other sizes above the ground are available on request.

For ground installation, three adjustable support feet, so that the instrument can be levelled correctly, and holes for fixing to the floor have been provided.

For raised installations, a collar to be fastened to the base of the instrument, and on which the support staff must be inserted, is provided. The staff may end with either a flange so that it can be fixed to the floor, or a tip to be driven into the ground. The various fastening systems can be seen in the figures 5, 6, 7 and 8.

For the tipping device to function correctly and so for the measurement to be correct, it is important that the instrument is placed perfectly levelled. The base of the rain gauge is fitted with a bubble level.

For installation, unscrew the three screws at the base of the cylinder that supports the water collector cone. **Attention:** a heating resistor is fitted around the cone in the **HD2013R** version. To disconnect the cone heater, unplug the connector on the upper side of the terminal block protection cover (see fig. 2).

## Electrical connection

For the version without heating use a 2-wire cable with 0.5 mm<sup>2</sup> minimum wires section, for the version with heating use a 4-wire cable with 2.5 mm<sup>2</sup> minimum wires section.

Use a shielded cable over long distances. Slide the cable through the cable gland and fasten it with the cable fastener located near the entry hole at the base of the rain gauge.

Unscrew the terminal block protection cover and perform the connections as shown in the following figures.

### Connection of heating:

The heated version requires power (12 Vdc or 24 Vdc depending on the version supplied) for the resistors: perform the connection as indicated at point 2 of fig. 2.

If the connections are set correctly, the LED placed near the terminals will be lit up.

### Connection of contact output:

The rain gauge contact output, indicated at point 1 in the figure 2, **must be connected to the input of the HD2013-DB rain gauge data logger** (please see the details in the manual of the data logger) **or to a pulse counter or to a data logger.**

To use the contact output in the versions with HD2013UA or HD2013UD option, set the SW1 switch down, towards the EXTERNAL indication (see the figures 3 and 4): the analog or SDI-12 output is disabled.

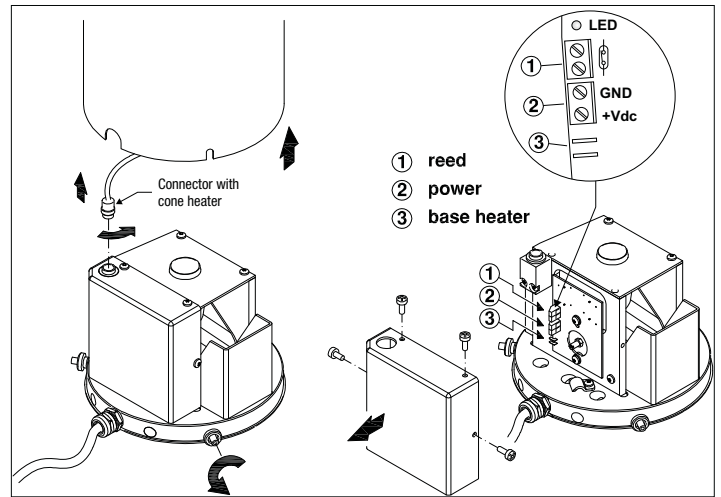


Fig. 2 – Connections of contact output and heating

### Connection of analog output (only with HD2013UA option):

Perform the connections as shown in figure 3. Set the SW1 switch up, towards the INTERNAL indication (the contact output is disabled).

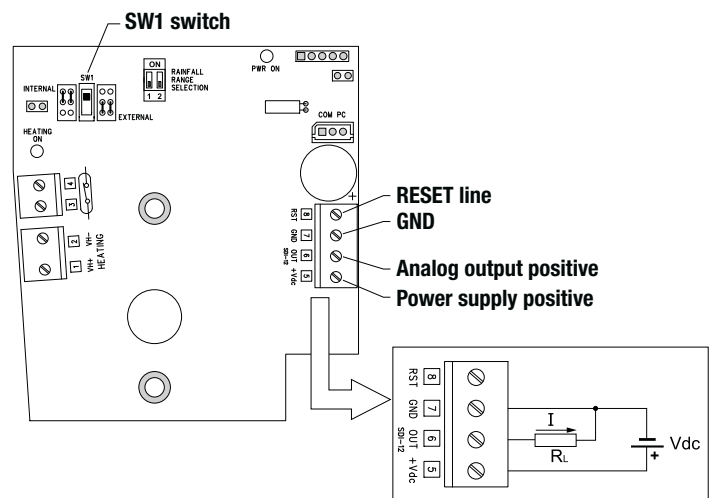


Fig. 3 – Connections of analog output

The current analog output is active. The maximum value of the load resistance depends on the power supply value:

$$R_L \text{ max} = 50 \times (V_{dc} - 7) \Omega$$

The minimum value of the load resistance for the version with voltage analog output is 10 KΩ.

In case of a measurement error, the analog output goes to the value 22 mA or 11 V.

The reset line allows the partial amount of rainfall measurement (amount of rainfall from the last reset command) to be remotely reset. During the measurement, the reset line must be connected to GND. To reset, disconnect the line from GND and apply a direct voltage of at least 3 Vdc (and lower than or equal to the power supply) for at least 1 s, then reconnect the line to GND.



Electrical connections

Connection of SDI-12 digital output (only with HD2013UD option):

Perform the connections as shown in figure 3. Set the SW1 switch up, towards the INTERNAL indication (the contact output is disabled).

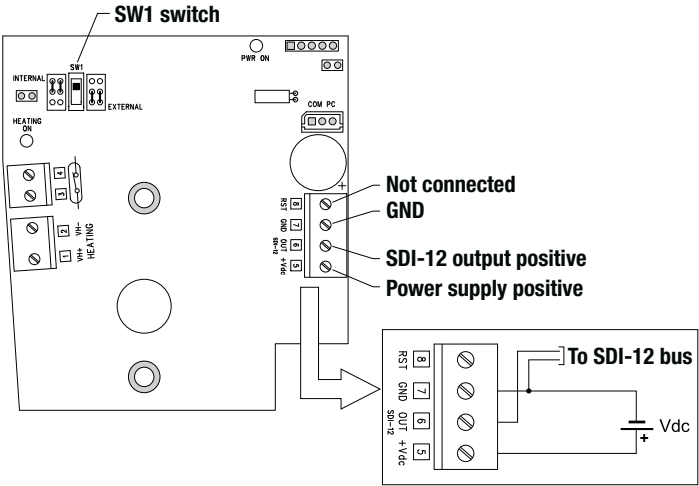


Fig. 4 – Connections of SDI-12 digital output

The reset line is not used in the version with digital output: the reset is performed with the appropriate SDI-12 extended command (**aRES!**, with **a**=address of the rain gauge).

Configuration of analog output

The analog output is proportional to the partial amount of rainfall (amount of rainfall from the last reset command). The analog output full scale (20 mA or 10 V) can be associated with different values of rainfall. The association can be implemented via hardware, by using the **dip switches** on the circuit board, or via software, by connecting the serial communication port **COM PC** of the rain gauge to the PC.

The dip switches allow setting three rainfall values: 25, 100 or 250 mm (1, 5 or 10 inches) if the set unit of measurement is “inches”), as shown in figure 5.

If both the dip switches are set to ON, the rainfall value considered is the one set via serial port with the command **CRW** (see the table of the serial commands).

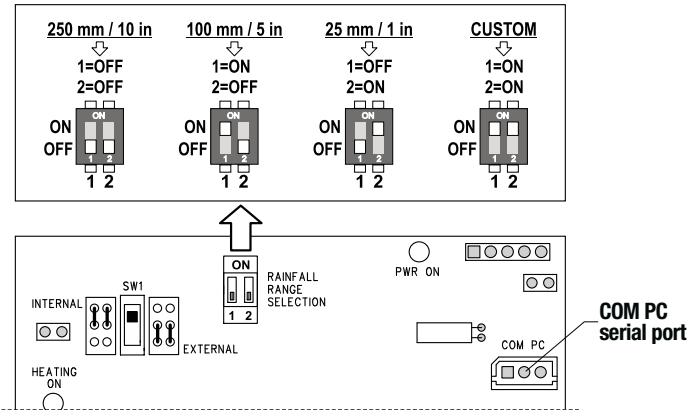


Fig. 5 – Dip switches

**Warning:** after reaching the full scale value, the measurement is reset and the analog output returns to the initial scale value.

Tipping bucket

The tipping bucket is locked for the transport of the rain gauge. To unlock the bucket, remove the holders as shown in fig. 6.

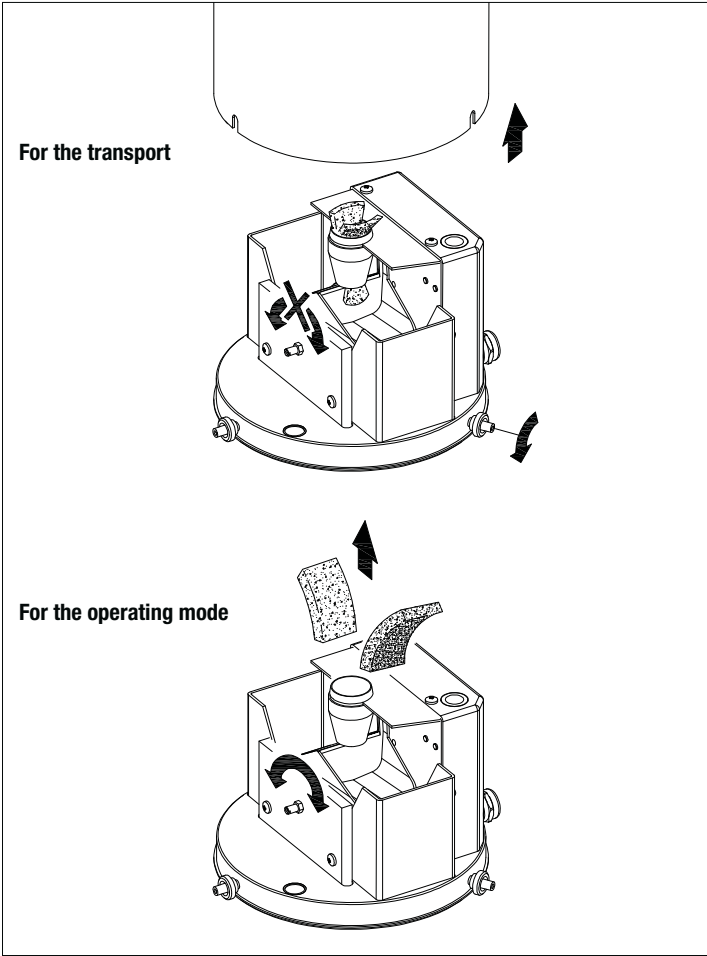


Fig. 6 – Locking and unlocking the tipping bucket

The oscillation of the tipping bucket can be adjusted through the two threaded rods located under the bucket, as illustrated in fig. 7.


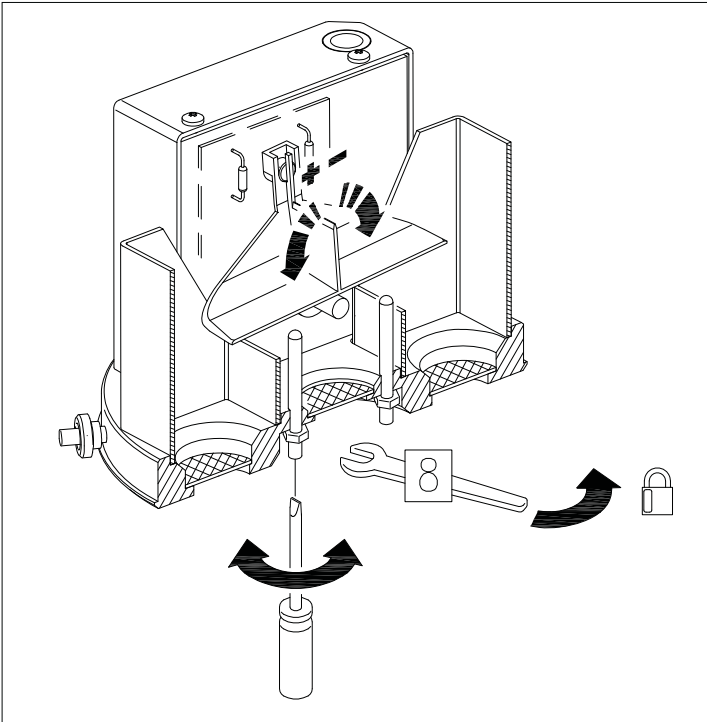


Fig. 7 – Adjustment of the tipping bucket



**Fig. 8 – Mechanical dimensions, installation modes**

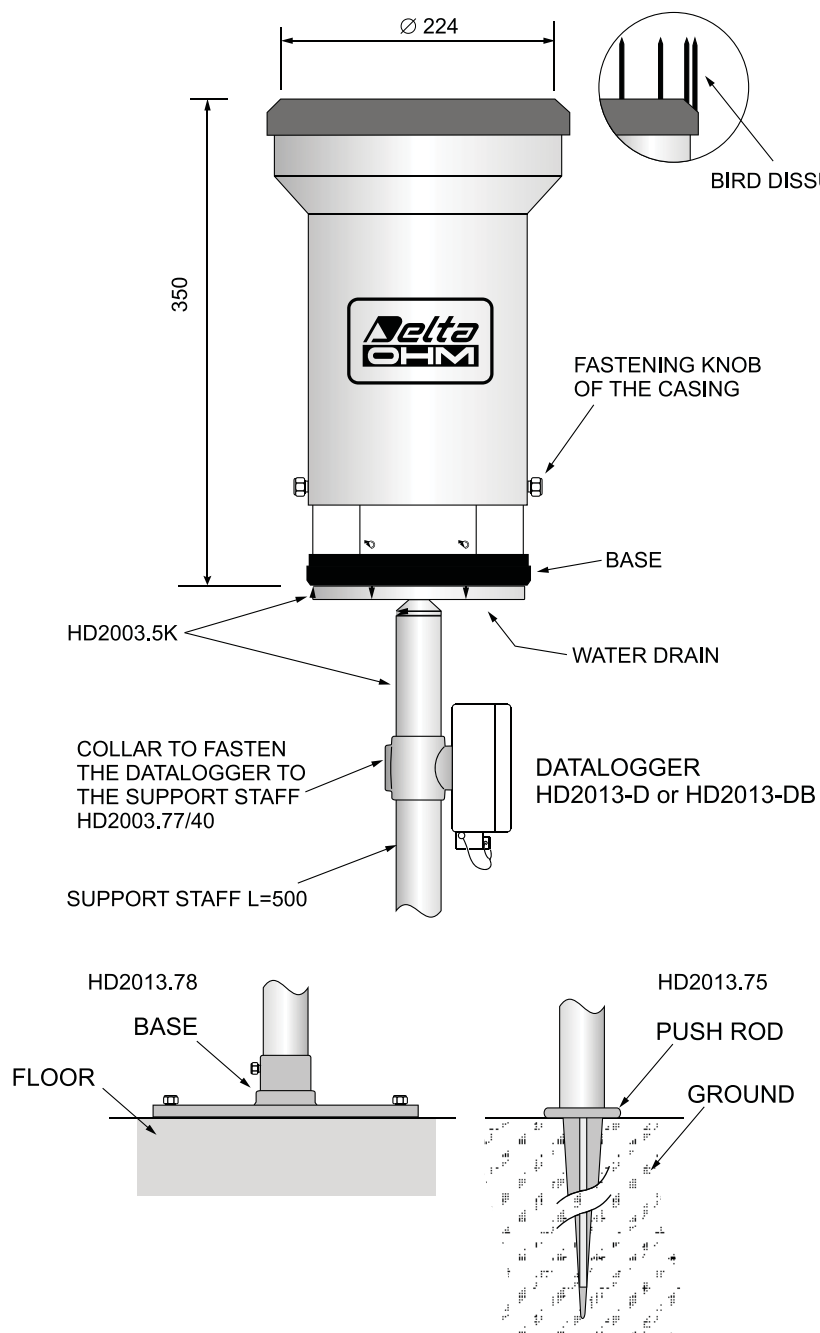


Bubble level




Rain gauge installed on the ground.




Rain gauge with bird dissuader.

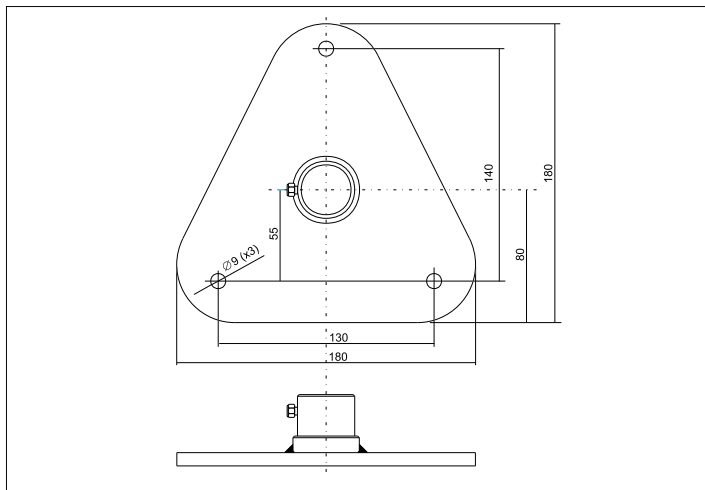

**Fig. 9 – Base for ground fastening (HD2013.78)**

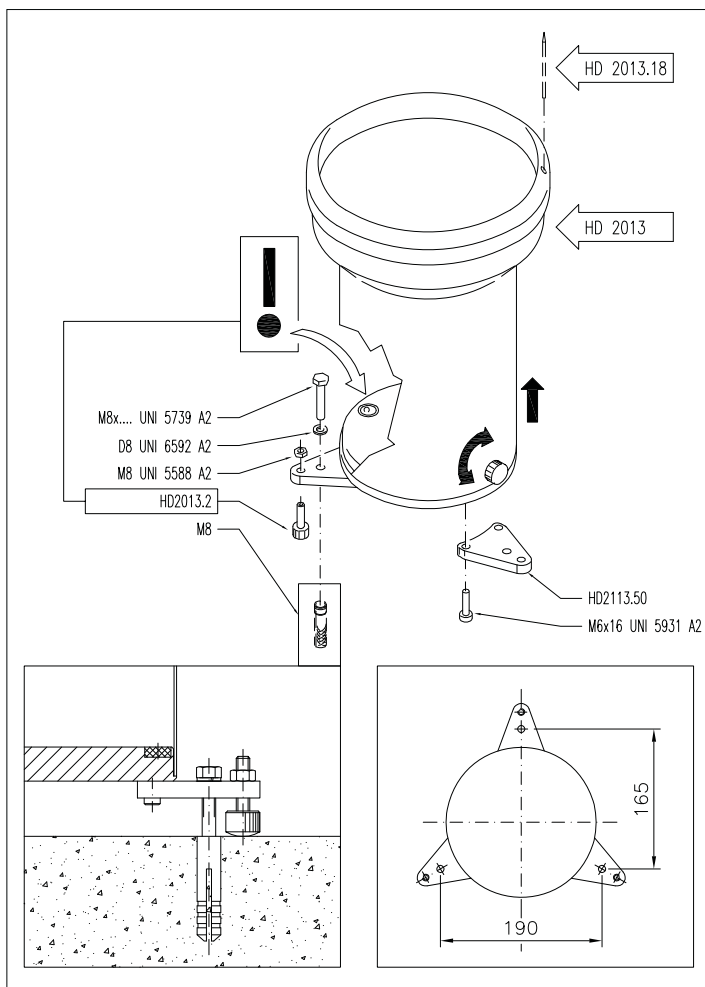

**Fig. 10 – Ground installation**

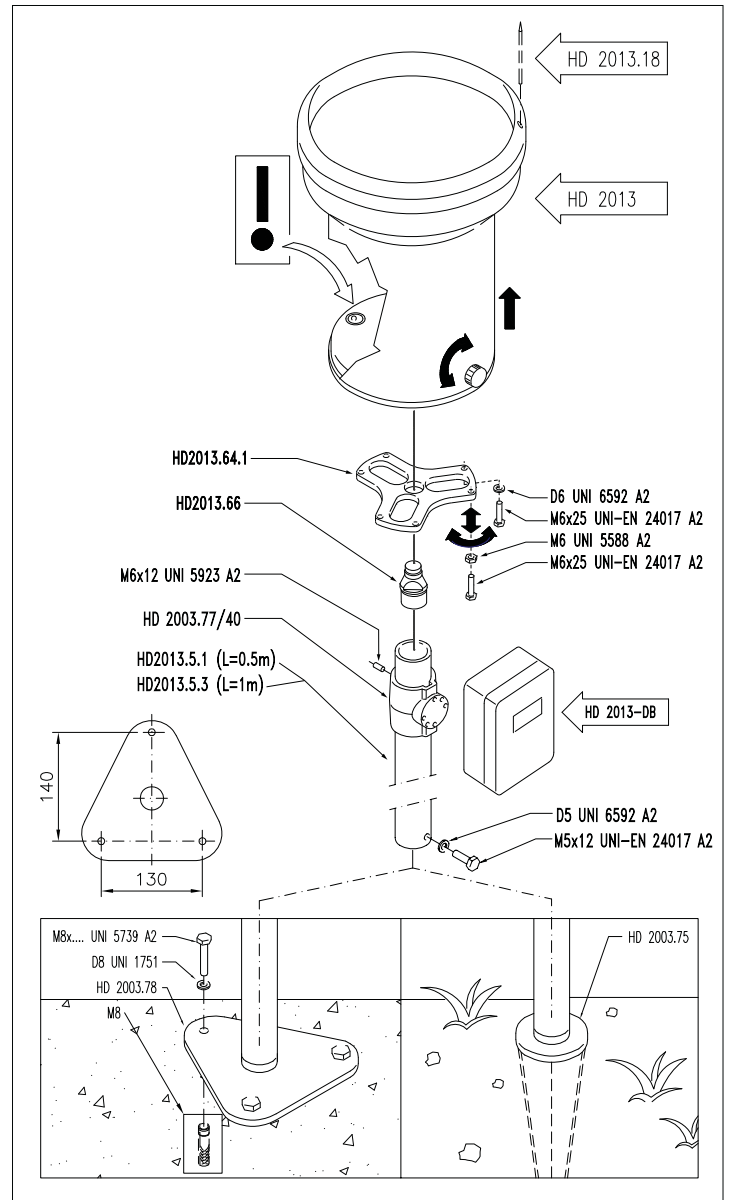

**Fig. 11 – Installation raised above ground**



Tip for ground for rain gauge raised from ground



Support plate for rain gauge raised from ground

## Serial commands

The rain gauges with HD2013UA or HD2013UD option allow editing or checking the operating parameters of the instrument via serial commands. Proceed as follows:

- Connect the serial port **COM PC** of the rain gauge to the RS232 (via the **RS27** cable) or USB (via the **CP27** cable) port of the PC. If the CP27 cable is used, install the corresponding USB drivers in your PC.
- In the PC, start a serial communication program (e.g. Hyperterminal), set the baud rate to 9600 and the communication parameters to 8N2.
- Send the commands given below to edit or check the value of the rain gauge parameters. In the editing commands, the new value of the parameter follows immediately (without spaces interposed) the command identifier.

The editing of the rain gauge parameters requires sending a password via the serial command **PWD**. By default, the password is not set; therefore, it is sufficient to send the command PWD without password to change the parameters. To protect the parameters from unauthorized changes, it is advisable to set a password with the serial command **SUP**. The password remains active for 10 minutes, after which you must resubmit it.

In the serial commands described below, the column "PWD" indicates whether the execution of the command is password protected.

## Password management

Command	Description	PWD
PWDx...x	Sends the password x...x (8 characters max.). Reply of the instrument: USER ACCESS OK if the password is accepted WRONG PASSWORD if the password is not accepted	---
SUPx...x	Sets the string x...x (8 ASCII characters max.) as password. Reply of the instrument: PASS: x...x if the password is accepted INVALID PASSWORD if the password is not accepted	Yes

## Date and time

Command	Description	PWD
DSyyyy/mm/dd hh:mm:ss	Sets the date yyyy/mm/dd (year/month/day) and the time hh:mm:ss (hour/minutes/seconds) in the rain gauge. Reply of the instrument: &l if date and time are accepted ? if date and time are not correct	Yes
DG	Reads the date (year/month/day) and the time (hour/minutes/seconds) set in the rain gauge. Reply of the instrument: yyyy/mm/dd hh:mm:ss	No

## General info

Command	Description	PWD
IR	Reads the manufacturer, the model, the firmware version and the serial number of the rain gauge. Reply of the instrument: v...vm...mf...fs...s, with: v...v (8 characters) = name of the manufacturer (DELTAOHM) m...m (6 characters) = model (HD2013) f...f (3 characters) = firmware version s...s (max. 13 characters) = serial number	No

## Unit of measurement

Command	Description	PWD
UWn	Sets the unit of measurement of index n for the amount of rainfall: n=0 ⇒ mm, n=1 ⇒ inches Reply of the instrument: &l if the unit of measurement is accepted ? if the index n is not correct	Yes
UR	Reads the unit of measurement of the amount of rainfall set in the rain gauge. Reply of the instrument: 0 if the unit of measurement is "mm" 1 if the unit of measurement is "inches"	No
TUWu	Sets the unit of measurement of the temperature <sup>(*)</sup> : u=C ⇒ °C, u=F ⇒ °F Reply of the instrument: &l if the unit of measurement is accepted ? if the character u is not correct	Yes
TUR	Reads the unit of measurement of the temperature <sup>(*)</sup> . Reply of the instrument: C if the unit of measurement is "°C" F if the unit of measurement is "°F"	No

<sup>(\*)</sup> The rain gauges with HD2013UA or HD2013UD option are equipped with a temperature sensor which detects the internal temperature of the instrument (**not the air temperature**). The temperature value can be read via the serial commands S1 / S2 or, in the rain gauges with HD2013UD option, via the appropriate SDI-12 command described in the paragraph "SDI-12 protocol".

## Resolution

Command	Description	PWD
BWn	Sets the rain gauge resolution (amount of rainfall corresponding to an emptying of the tipping bucket) of index n:  n=0 ⇒ 0.1 mm n=1 ⇒ 0.2 mm n=2 ⇒ 0.25 mm n=3 ⇒ 0.5 mm n=4 ⇒ 1.0 mm n=5 ⇒ 0.254 mm (0.01 inches) n=6 ⇒ 0.508 mm (0.02 inches) n=7 ⇒ 1.016 mm (0.04 inches) n=X ⇒ custom value (set via the CCW command)  Reply of the instrument: &l if the resolution is accepted ? if the index n is not correct	Yes
BR	Reads the rain gauge resolution.  The reply of the instrument is the index n of the resolution according to the list given in the description of the editing command BW.	No
CCWn...n	Sets n...n as custom value of the resolution. The value must be between 0.001 and 10.00 and is considered in the unit of measurement (mm or inches) set in the instrument.  Example: CCW+0.42 sets 0.42 mm or 0.42 inches, depending on the unit of measurement set, as custom value of the resolution.  Reply of the instrument: &l if the value n...n is accepted ? if the value n...n is not correct  <i>Warning:</i> the command CCW sets the value but not the use of the custom resolution; to use the custom resolution, the command BWX should be sent (see the command BW described above).	Yes
CCR	Reads the custom value of the resolution. The value is considered in the unit of measurement (mm or inches) set in the instrument.	No

## Output contact type

Command	Description	PWD
TNWn	Sets the rain gauge output contact as normally open or normally closed: n=0 ⇒ Normally CLOSED, n=1 ⇒ Normally OPEN  Reply of the instrument: &l if the setting is accepted ? if the index n is not correct	Yes
TNR	Reads the type of the rain gauge output contact.  Reply of the instrument: 0 if the contact is normally CLOSED 1 if the contact is normally OPEN	No



## Analog output (only with HD2013UA option)

Command	Description	PWD
CPOE	Enables the offset of the analog output initial value: 4...20 mA or 2...10 V. Reply of the instrument: &l	Yes
CPOD	Disables the offset of the analog output initial value: 0...20 mA or 0...10 V. Reply of the instrument: &l	Yes
CPOR	Reads the enabling state of the offset of the analog output initial value. Reply of the instrument: 0 if the offset is disabled (0...20 mA or 0...10 V) 1 if the offset is enabled (4...20 mA or 2...10 V)	No
CRWn...n	Sets n...n as the amount of rainfall corresponding to the analog output full scale. The value must be between 0.01 and 9999.00 and is considered in the unit of measurement (mm or inches) set in the instrument. Example: CRW+80.00 sets 80 mm or 80 inches, depending on the unit of measurement set, as value corresponding to 20 mA or 10 V. Reply of the instrument: &l if the value n...n is accepted ? if the value n...n is not correct	Yes
CRR	Reads the amount of rainfall corresponding to the analog output full scale. The value is considered in the unit of measurement (mm or inches) set in the instrument.	No

## Printing of the measurements (only with HD2013UA option)

Command	Description	PWD
S0	Stops the continuous printing of the measurements. Reply of the instrument: &l	No
S1	Single printing of the measurement values, considered in the unit of measurement set in the instrument. Reply of the instrument: + $M_1$ + $M_2$ + $M_3$ + $M_4$ + $M_5$ , with: $M_1$ = total amount of rainfall (from when the instrument is powered) $M_2$ = partial amount of rainfall (from the last reset operation) $M_3$ = amount of rainfall in the current day $M_4$ = amount of rainfall in the previous day $M_5$ = internal temperature of the rain gauge Example: the reply +873.4+15.8+2.6+3.4+12.5 indicates that the amount of rainfall is: 873,4 mm or inches from when the instrument is powered 15,8 mm or inches from the last reset operation 2,6 mm or inches today 3,4 mm or inches yesterday In addition, the rain gauge internal temperature is 12.5 °C or °F. Note: after reaching 99999.99, the total rainfall counter restarts from zero.	No
S2	Continuous printing (once per second) of the measurement values, considered in the unit if measurement set in the instrument. The reply of the instrument is in the same form described for the command S1.	No

## Reset

Command	Description	PWD
RES	Resets the partial rainfall counter. Reply of the instrument: &l	Yes
HRS	Resets the electronic board (with consequent reset of all the measuring counters).	Yes

## Correction of the measurement

To increase the measurement accuracy, a measurement correction table as a function of the rainfall rate can be stored in the rain gauge.

The correction is useful because during the emptying time of the tipping bucket, rain is not collected from the bucket and the amount of rain in the absence of correction is therefore underestimated. The correction to be made is greater the higher is the rainfall rate (greater number of cycles in the time unit).

The rain gauge allows you to set ten multiplication factors (numbered from 0 to 9) of the nominal resolution, each corresponding to a range of rainfall rate.

By default, the multiplication factors are all set to 1. **As option, you can request that the correction factors of the specific rain gauge are already stored.**

Command	Description	PWD
TE	Enables the measurement correction as a function of the rainfall rate. Reply of the instrument: &l	Yes
TD	Disables the measurement correction as a function of the rainfall rate. Reply of the instrument: &l	Yes
TR	Reads the enabling state of the measurement correction as a function of the rainfall rate. Reply of the instrument: 0 if the correction is disabled 1 if the correction is enabled	No
CTS	Starts the correction table writing procedure. Reply of the instrument: CALIBRATION_STARTED	Yes
CTE	Ends the correction table writing procedure and saves the entered values. Reply of the instrument: CALIBRATION_ENDED	Yes
CTWi+r...r+k...k	Set the multiplication factor of index $i$ to the value $k...k$ . The multiplication factor is applied if the rainfall rate is between $r...r$ (considered in mm/h or in/h depending on the unit of measurement set in the instrument) and the rate value defined for the multiplication factor of index $i+1$ (see the example below). The multiplication factor must be between 0.500 and 2.000. The rainfall rate must be between 0 and 7200. Reply of the instrument: &l if the parameters are correct ? if the parameters are not correct	Yes
CTR <i>i</i>	Reads the setting of the multiplication factor of index $i$ . Reply of the instrument: $r...rk...k$ , with: $r...r$ = rainfall rate corresponding to the multiplication factor $k...k$ = value of the multiplication factor Example: +50+1.05 indicates that the multiplication factor is 1.05 and the corresponding rainfall rate is 50 (mm/h or in/h).	No

When you set the correction table, it is mandatory to enter in ascending order all the ten multiplication factors. The rate corresponding to the multiplication factor of index  $i$  must be greater or equal to the rate corresponding to the multiplication factor of index  $i-1$ .

**Example:** to implement the following correction table:

Rainfall rate (mm/h)										
	0...25	25...50	50...75	75...90	90...120	120...150	150...180	180...220	220...260	260...
<b>K</b>	1	1.02	1.04	1.06	1.08	1.1	1.12	1.15	1.18	1.2

send, exactly in the order shown, the following commands:

CTS  
CTW0+0+1  
CTW1+25+1.02  
CTW2+50+1.04  
CTW3+75+1.06  
CTW4+90+1.08  
CTW5+120+1.1  
CTW6+150+1.12  
CTW7+180+1.15  
CTW8+220+1.18  
CTW9+260+1.2  
CTE

Note that the sequence of the CTW commands must be preceded by the command CTS and followed by the command CTE.



## SDI-12 protocol

The rain gauge with **HD2013UD** option is equipped with an SDI-12 communication interface compliant with the version 1.3 of the protocol, which allows the connection to SDI-12 sensor networks.

The communication parameters of the PC or of the data logger should be set as follows:

baud rate: 1200, data bits: 7, parity: Even, stop bits: 1

The communication with the instrument is performed by generating a *Break signal* on the serial line for at least 12 ms (the function that generates the Break signal is usually available in programming languages or in serial communication programs) and then by sending a command in the following form:

**<Address><Command>!**

with <Address> = address of the instrument the command is sent to

<Command> = type of operation requested to the instrument

The instrument reply is as follows:

**<Address><Data><CR><LF>**

with <Address> = address of the instrument which replies

<Data> = information sent by the instrument

<CR> = ASCII character *Carriage Return*

<LF> = ASCII character *Line Feed*

The rain gauge comes with a factory address preset to 0. The address can be modified by using the proper SDI-12 command reported in the following table.

The following table reports the SDI-12 commands available. To comply with the SDI-12 standard, the instrument address is indicated in the table with the letter **a**.

## SDI-12 Commands

Command	Instrument reply	Description
<b>a!</b>	a<CR><LF>	Verifies the presence of the instrument.
<b>all</b>	allccccccmmmmmmvvvsssssss<CR><LF> with: a = address of the instrument (1 character) ll = SDI-12 compliant version (2 characters) cccccc = manufacturer (8 characters) mmmmmm = instrument model (6 characters) vvv = firmware version (3 characters) sssssss = serial number (8 characters)  ⇒ Example of response: 013Delta0hm HD201310013201518 with: 0 = instrument address 13 = SDI-12 version 1.3 compliant Delta0hm = manufacturer's name HD2013 = instrument model 100 = firmware version 1.0.0 13201518 = serial number	Requests for information from the instrument.
<b>aAb!</b> Where: b = new address	b<CR><LF> Note: if the b character is not an acceptable address, the instrument responds with a instead of b.	Modification of the instrument address.
<b>?! </b>	a<CR><LF>	Request of the address of the instrument. If more than one sensor is connected to the bus, a conflict occurs.
<b>TYPE M COMMANDS (START MEASUREMENT)</b>		
<b>Total amount of rainfall</b>		
<b>aM!</b>	atttn<CR><LF> with: ttt = number of seconds necessary for the instrument to make the measure available (3 characters) n = number of detected variables (1 character) Note: ttt = 000 means that datum is immediately available.	Request of detection of the total amount of rainfall (from when the instrument is powered).
<b>aDO!</b>	a+n+r...r<CR><LF> with: n = number of emptying of the tipping bucket r...r = total amount of rainfall in the unit of measurement set in the instrument (mm or inches)  ⇒ Example of response: 0+48+9.6 The instrument with address 0 has recorded 48 emptying of the tipping bucket and the total amount of rainfall is 9.6 mm or inches depending on the set unit. Note: after reaching 99999.99, the total rainfall counter restarts from zero.	Reads the total amount of rainfall (from when the instrument is powered).

Command	Instrument reply	Description
<b>Partial amount of rainfall</b>		
<b>aM1!</b>	atttn<CR><LF> with: ttt = number of seconds necessary for the instrument to make the measure available (3 characters) n = number of detected variables (1 character) Note: ttt = 000 means that datum is immediately available.	Request of detection of the partial amount of rainfall (from the last reset command).
<b>aDO!</b>	a+n+r...r<CR><LF> with: n = number of emptying of the tipping bucket r...r = partial amount of rainfall in the unit of measurement set in the instrument (mm or inches)  ⇒ Example of response: 0+12+2.4 The instrument with address 0 has recorded 12 emptying of the tipping bucket and the partial amount of rainfall is 2.4 mm or inches depending on the set unit.  Note: after reaching 99999.99, the partial rainfall counter restarts from zero.	Reads the partial amount of rainfall (from the last reset command).
<b>Amount of rainfall in the current day</b>		
<b>aM2!</b>	atttn<CR><LF> with: ttt = number of seconds necessary for the instrument to make the measure available (3 characters) n = number of detected variables (1 character) Note: ttt = 000 means that data are immediately available.	Request of detection of the amount of rainfall in the current day.
<b>aDO!</b>	a+n+r...r<CR><LF> with: n = number of emptying of the tipping bucket r...r = amount of rainfall in the current day in the unit of measurement set in the instrument (mm or inches)  ⇒ Example of response: 0+2+0.4 The instrument with address 0 has recorded 2 emptying of the tipping bucket and the amount of rainfall today is 0.4 mm or inches depending on the set unit.	Reads the amount of rainfall in the current day.
<b>Amount of rainfall in the previous day</b>		
<b>aM3!</b>	atttn<CR><LF> with: ttt = number of seconds necessary for the instrument to make the measure available (3 characters) n = number of detected variables (1 character) Note: ttt = 000 means that data are immediately available.	Request of detection of the amount of rainfall in the previous day.
<b>aDO!</b>	a+n+r...r<CR><LF> with: n = number of emptying of the tipping bucket r...r = amount of rainfall in the previous day in the unit of measurement set in the instrument (mm or inches)  ⇒ Example of response: 0+8+1.6 The instrument with address 0 has recorded 2 emptying of the tipping bucket and the amount of rainfall yesterday was 1.6 mm or inches depending on the set unit.	Reads the amount of rainfall in the previous day.
<b>Rainfall rate</b>		
<b>aM4!</b>	atttn<CR><LF> with: ttt = number of seconds necessary for the instrument to make the measure available (3 characters) n = number of detected variables (1 character) Note: ttt = 000 means that data are immediately available.	Request of detection of the current rainfall rate.
<b>aDO!</b>	a+r...r<CR><LF> with: r...r = rainfall rate in the unit of measurement set in the instrument (mm/h or in/h)  ⇒ Example of response: 0+7.3 The instrument with address 0 measures a rate of 7.3 mm/h or in/h depending on the set unit.	Reads the current rainfall rate.

Command	Instrument reply	Description
<b>Power supply voltage and internal temperature</b>		
<b>aM5!</b>	atttn<CR><LF> with: ttt = number of seconds necessary for the instrument to make the measures available (3 characters) n = number of detected variables (1 character) Note: ttt = 000 means that data are immediately available.	Request of detecting the power supply voltage and the internal temperature of the rain gauge.
<b>aD0!</b>	a+v...v+t...t<CR><LF> with: v...v = power supply voltage in V t...t = internal temperature in the unit of measurement set in the instrument (°C or °F) ⇒ Example of response: 0+15.3+0 The instrument with address 0 has 12.0 power supply voltage and 15.3 °C internal temperature (if °C is the set unit).	Reads the power supply voltage and the internal temperature of the rain gauge.
<b>TYPE C COMMANDS (START CONCURRENT MEASUREMENT)</b>		
<b>Total amount of rainfall</b>		
<b>aC!</b>	atttn<CR><LF> with: ttt = number of seconds necessary for the instrument to make the measure available (3 characters) n = number of detected variables (1 character) Note: ttt = 000 means that datum is immediately available.	Request of detection of the total amount of rainfall (from when the instrument is powered).
<b>aD0!</b>	a+n+r...r<CR><LF> with: n = number of emptying of the tipping bucket r...r = total amount of rainfall in the unit of measurement set in the instrument (mm or inches)	Reads the total amount of rainfall (from when the instrument is powered).
<b>Partial amount of rainfall</b>		
<b>aC1!</b>	atttn<CR><LF> with: ttt = number of seconds necessary for the instrument to make the measure available (3 characters) n = number of detected variables (1 character) Note: ttt = 000 means that datum is immediately available.	Request of detection of the partial amount of rainfall (from the last reset command).
<b>aD0!</b>	a+n+r...r<CR><LF> with: n = number of emptying of the tipping bucket r...r = partial amount of rainfall in the unit of measurement set in the instrument (mm or inches)	Reads the partial amount of rainfall (from the last reset command).
<b>Amount of rainfall in the current day</b>		
<b>aC2!</b>	atttn<CR><LF> with: ttt = number of seconds necessary for the instrument to make the measure available (3 characters) n = number of detected variables (1 character) Note: ttt = 000 means that data are immediately available.	Request of detection of the amount of rainfall in the current day.
<b>aD0!</b>	a+n+r...r<CR><LF> with: n = number of emptying of the tipping bucket r...r = amount of rainfall in the current day in the unit of measurement set in the instrument (mm or inches)	Reads the amount of rainfall in the current day.
<b>Amount of rainfall in the previous day</b>		
<b>aC3!</b>	atttn<CR><LF> with: ttt = number of seconds necessary for the instrument to make the measure available (3 characters) n = number of detected variables (1 character) Note: ttt = 000 means that data are immediately available.	Request of detection of the amount of rainfall in the previous day.
<b>aD0!</b>	a+n+r...r<CR><LF> with: n = number of emptying of the tipping bucket r...r = amount of rainfall in the previous day in the unit of measurement set in the instrument (mm or inches)	Reads the amount of rainfall in the previous day.

Command	Instrument reply	Description
<b>Rainfall rate</b>		
<b>aC4!</b>	atttn<CR><LF> with: ttt = number of seconds necessary for the instrument to make the measure available (3 characters) n = number of detected variables (1 character) Note: ttt = 000 means that data are immediately available.	Request of detection of the current rainfall rate.
<b>aD0!</b>	a+r...r<CR><LF> with: r...r = rainfall rate in the unit of measurement set in the instrument (mm/h or in/h)	Reads the current rainfall rate.
<b>Power supply voltage and internal temperature</b>		
<b>aC5!</b>	atttn<CR><LF> with: ttt = number of seconds necessary for the instrument to make the measures available (3 characters) n = number of detected variables (1 character) Note: ttt = 000 means that data are immediately available.	Request of detecting the power supply voltage and the internal temperature of the rain gauge.
<b>aD0!</b>	a+v...v+t...t<CR><LF> with: v...v = power supply voltage in V t...t = internal temperature in the unit of measurement set in the instrument (°C or °F)	Reads the power supply voltage and the internal temperature of the rain gauge.
<b>TYPE R COMMAND (CONTINUOUS MEASUREMENTS)</b>		
<b>aR0!</b>	a+n+r...r<CR><LF> with: n = number of emptying of the tipping bucket r...r = total amount of rainfall in the unit of measurement set in the instrument (mm or inches)	Reads the total amount of rainfall (from when the instrument is powered).
<b>aR1!</b>	a+n+r...r<CR><LF> with: n = number of emptying of the tipping bucket r...r = partial amount of rainfall in the unit of measurement set in the instrument (mm or inches)	Reads the partial amount of rainfall (from the last reset command).
<b>aR2!</b>	a+n+r...r<CR><LF> with: n = number of emptying of the tipping bucket r...r = amount of rainfall in the current day in the unit of measurement set in the instrument (mm or inches)	Reads the amount of rainfall in the current day.
<b>aR3!</b>	a+n+r...r<CR><LF> with: n = number of emptying of the tipping bucket r...r = amount of rainfall in the previous day in the unit of measurement set in the instrument (mm or inches)	Reads the amount of rainfall in the previous day.
<b>aR4!</b>	a+r...r<CR><LF> with: r...r = rainfall rate in the unit of measurement set in the instrument (mm/h or in/h)	Reads the current rainfall rate.
<b>aR5!</b>	a+v...v+t...t<CR><LF> with: v...v = power supply voltage in V t...t = internal temperature in the unit of measurement set in the instrument (°C or °F)	Reads the power supply voltage and the internal temperature of the rain gauge.

In addition to the above-mentioned commands, the rain gauge also implements the corresponding commands with CRC, that require to add a 3-character CRC code at the end of the reply before <CR><LF>. The format of these commands is obtained from the previous by adding the letter C: aMC1, aMC1!, aMC2!, aMC3!, aMC4, aMC5!, aCC1, aCC1!, aCC2!, aCC3!, aCC4!, aCC5!, aRC0!, aRC1!, aRC2!, aRC3!, aRC4!, aRC5!

### SDI-12 extended commands

In addition to the standard SDI-12 commands, the rain gauge with HD2013UD option has extended commands that allow you to configure the instrument also via the SDI-12 line, as an alternative to the configuration via the serial port COM PC. The extended commands are those already described in the paragraph "Serial commands", with the difference that they must be preceded by the address of the instrument they are sent to, and must end with the character ! (exclamation mark).

For example, to set °F as temperature unit of measurement in the instrument with address 0, send:

OPWDMypass!      Sends the password (assuming password=mypass)  
OTUWF!              Sets °F

The reply to an extended command is always preceded by the address of the instrument that replies.

## Maintenance

Verify filter cleanliness periodically; check that there is no debris, leaves, dirt in the lower filter or anything else that might obstruct the flowing of water. Check that the tipping bucket contains no deposits of dirt, sand or any other obstruction. If necessary, the surfaces can be cleaned with non aggressive detergent.


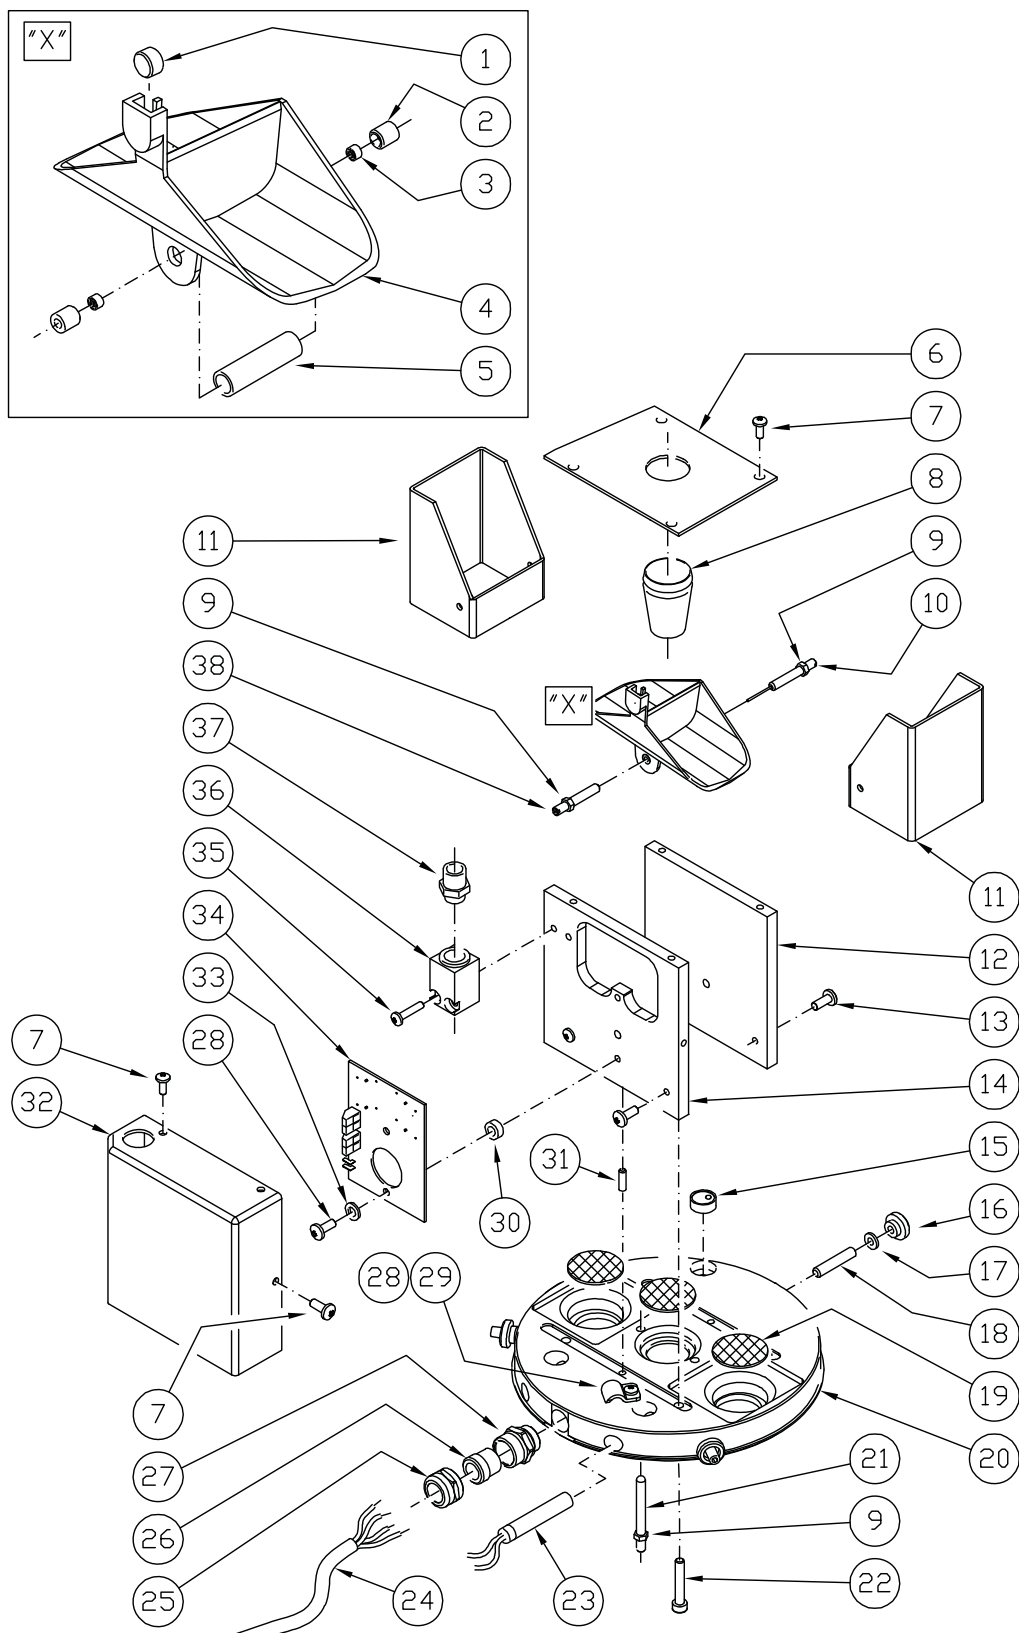


Fig. 12 – Exploded view of the lower part (version with heating)

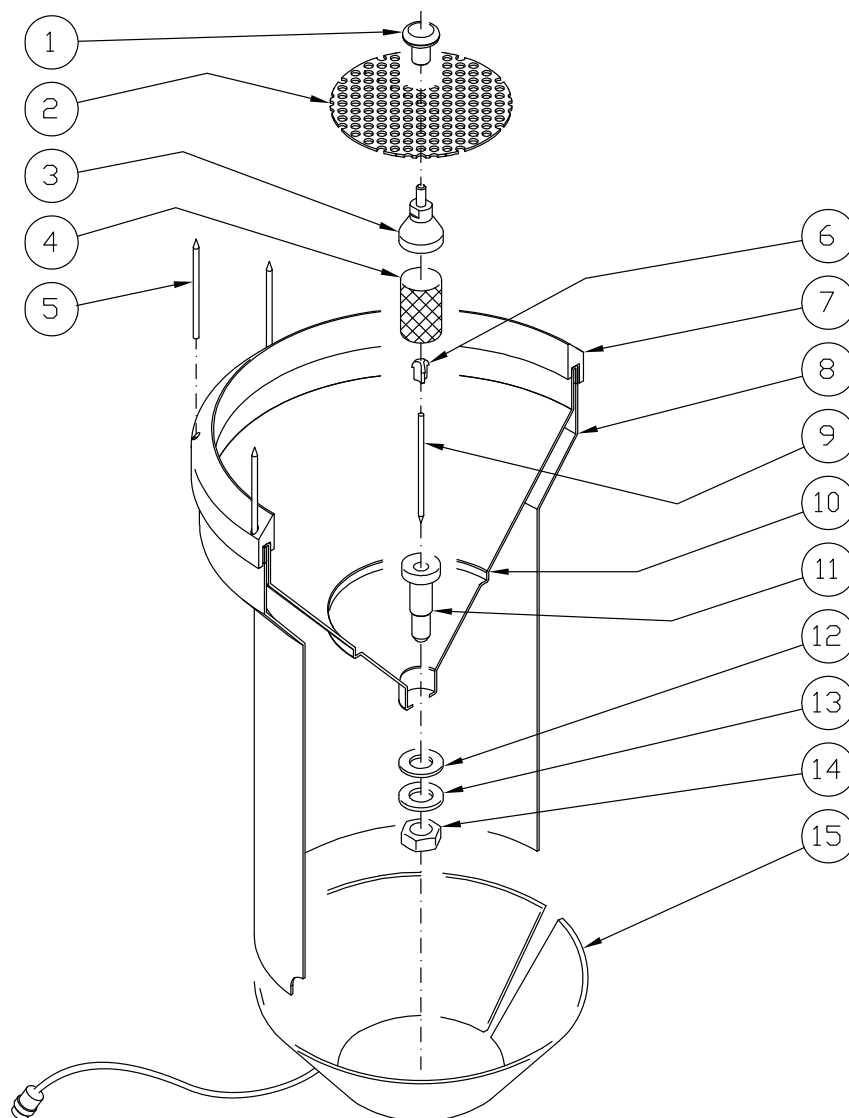

**Fig. 13 – Exploded view of the upper part (version with heating)**

## Order codes

<b>HD2013</b>	Tipping bucket rain gauge, area 400 cm <sup>2</sup> , for temperatures from +4 °C to +60 °C; resolution on request when ordering 0.1 – 0.2 or 0.5 mm. Output contact normally closed.
<b>HD2013R</b>	Tipping bucket rain gauge, area 400 cm <sup>2</sup> , with heating for temperatures from -20 °C to +60 °C. Resolution on request at the time of placing the order 0.1 – 0.2 or 0.5 mm. Output contact normally closed. Power supply voltage: 12 Vdc or 24 Vdc ± 10% (to be specified when ordering) / absorbed power 165W.
<b>HD2013UA</b>	Option HD2013 rain gauge with contact output and analog output at choice between 4...20 mA or 0...10 Vdc (to be specified when ordering). Power supply 7...30 Vdc for 4...20 mA output, 13...30 Vdc for 0...10 Vdc output.
<b>HD2013UD</b>	Option HD2013 rain gauge with contact output and SDI-12 digital output. Power supply 7...30 Vdc.
<b>HD2013.18</b>	Bird dissuader.
<b>HD2013.5K</b>	Accessory kit for the installation of the rain gauge raised 500 mm from ground (HD2003.78 + HD2013.5.1 + HD2013.64.1 + HD2013.66).
<b>HD2013.5K.1</b>	Accessory kit for the installation of the rain gauge raised 1 m from ground (HD2003.78 + HD2013.5.3 + HD2013.64.1 + HD2013.66).
<b>HD2013.75</b>	Base with tip for the ground to support the rain gauge raised above ground.
<b>HD2013.78</b>	Flat base for fastening the support of the rain gauge raised above ground.





## MANUFACTURE OF PORTABLE, BENCH TOP AND PROCESS SCIENTIFIC INSTRUMENTS

Current and voltage loop transmitters and regulators

Temperature - Humidity, Dew point - Pressure - CO, CO<sub>2</sub>

Air speed - Light - Optical Radiation

Acoustics - Vibration

Data logger - Data logger wireless

Microclimate

pH - Conductivity - Dissolved Oxygen - Turbidity

Elements for weather stations



**ACCREDIA**  
L'ENTE ITALIANO DI ACCREDITAMENTO

LAT N° 124 Signatory of EA, IAF and ILAC Mutual Recognition Agreements

Temperature - Humidity - Pressure - Air speed

Photometry/Radiometry - Acoustics

### CE CONFORMITY

- **Safety:** EN61000-4-2, EN61010-1 Level 3
- **Electrostatic discharge:** EN61000-4-2 Level 3
- **Electric fast transients:** EN61000-4-4 Level 3, EN61000-4-5 Level 3
- **Voltage variations:** EN61000-4-11
- **Electromagnetic interference susceptibility:** IEC1000-4-3
- **Electromagnetic interference emission:** EN55022 class B



Delta Ohm srl

Via G. Marconi, 5

35030 Caselle di Selvazzano (PD) - Italy

Tel. 0039 0498977150 r.a.

Fax 0039 049635596

e-mail: [info@deltaohm.com](mailto:info@deltaohm.com)

Web Site: [www.deltaohm.com](http://www.deltaohm.com)



Made in Italy

01  
06.15